

Weqas
Unit 6, Parc Tŷ Glas
Llanishen, Cardiff, CF14 5DU

Tel: 02920 314750
Fax: 02920 314760
Email: contact@weqas.com



EXTERNAL
QUALITY
ASSESSMENT



INTERNAL
QUALITY
CONTROL



REFERENCE
MEASUREMENT
SERVICES



EDUCATION &
TRAINING


Weqas

GLOBAL PROVIDER OF QUALITY
IN DIAGNOSTIC MEDICINE


Analytical interferences due to sample integrity Weqas Serum indices Programme – a 10 year journey

Annette Thomas


Haemolysis is the release of intracellular components from erythrocytes and other blood cells into the extra cellular fluid and can be caused by inappropriate or incorrect sample processing. Even if hemolysis is not visible there may still be discharge of cellular contents into the serum/plasma. At haemoglobin concentrations exceeding 300 mg/l (18.8 mmol/l), haemolysis is visible to the eye by the red colour of the plasma. Haemolyzed samples are a rather frequent occurrence in laboratory practice, with a prevalence as high as 3.3% and accounting for nearly 60% of rejected samples.



Lipaemia is turbidity of the sample due to the presence of triglyceride. It can be detected visually if the concentration of triglycerides in patient samples is over 300 mg/dl (3.4 mmol/L). Lipaemic samples cannot be avoided as increased concentration of lipids is often secondary to other disease states such as: diabetes mellitus, ethanol use, chronic renal failure and pancreatitis etc.



Icterus is the term given to elevated concentrations of bilirubin. Such elevations can be found in a variety of conditions including acute and chronic liver disease, biliary cirrhosis, alcoholism or as a physiological response to many drugs. The visual recognition of hyperbilirubinemia is often not sufficiently sensitive. Because of the high absorbance of bilirubin within the range 340 to 500 nm and the high background, the linearity range of the method can become a limiting factor for spectrophotometric analyses at these wavelengths.



Pre-analytical errors due to sample interferences: A WEQAS study to monitor the effectiveness of serum indices and Bilirubin interference.

In late 2010 users of the Weqas Serum Chemistry programme were provided with challenging samples containing either bilirubin, haemoglobin or triglyceride. The aim of the studies were to assess:

- the ability of the analysers Haemolytic / Icteric / Lipaemic (HIL) indices test to identify the presence of these potential interference.
- how laboratories deal with results where indices suggest that interferences are present in the sample.
- the interference effects of these parameters on the respective methods in routine use.



Samples were spiked with conjugated and unconjugated bilirubin to provide total bilirubin covering a range of 60- 500 µmol/L, Intralipid to a triglyceride range of 3 to 12.6 mmol/L and whole blood to provide a haemoglobin range of 0.4 to 3g/L. Two matched pools were distributed, one containing the interferant and the other the base serum.

In 2020, a separate stand alone serum indices programme was launched. Over 200 users now report results with the majority using semi-quantitative methods.

Quant Mean	IQN		IQQ		IQT		IQW		IQZ	
	H		I		L		I		L	
Analysers	0.3g/L		52 µmol/L		6.3 mmol/L		347 µmol/l		3.6 mmol/L	
Analysers	Results	No.	Results	No.	Results	No.	Results	No.	Results	No.
Interpretation	+		+		+++		+++		++	
Advia	Neg/- (0-0.22)	12	Neg, -	1	Neg,-		Neg,-	2	Neg,-	
	+ (0.23-1.0)	1	+	26	+		+		+	
	++ (1.1-2.33)		++		++		++	6	++	29
	+++ (2.34-3.78)		+++		+++	27	+++	22	+++	
	++++ (3.79 ->)		++++		++++		++++		++++	1
% correct	8%		96%		100%		73%		97%	
Interpretation	+/0.5-0.99		+		++++		+++		+++	
Beckman AU	Neg/- /<0.5		Neg, -	29	Neg,-	2	Neg,-		Neg,-	
	+ /0.5-0.99	24	+	12	+		+		+	
	+/1.00-1.99		++		++		++		++	1
	++/2.00-2.99		+++		+++		+++	47	+++	25
	+++/3.00-5.00		++++		++++	23	++++	1	++++	9
% correct	100%		29%		55%		98%		71%	
Interpretation	1 – 2/0.0-0.75		2-4		9-10		11-17		6 - 8	
Beckman DX	Neg/0		Neg, 0-1		Neg, 0-1		Neg, 0-1		Neg, 0-1	
	1 – 2 (0.0-0.75)	3	2-4	5	2		2-4		2	
	3 – 4 (0.75-1.50)		5-10		3-5		5-10		3 - 5	1
	5 – 6 (1.50-2.25)		11-17		6-8		11-17	5	6 - 8	4
	7 – 8 (2.25-2.75)		18-20		9-10	5	18-20		9 - 10	
9 – 10 (2.75-3.50)										
% correct	100%		100%		100%		100%		80%	
Interpretation			+		+++		+++		+++	
Piccolo	Neg/-		Neg/-	5	Neg,-		Neg,-		Neg,-	
	+		+		+		+		+	
	++		++		++		++		++	
	+++		+++		+++	4	+++	3	+++	6
% correct			0%		100%		100%		100%	

Assay Interferences

The early studies showed that for the icteric samples, method interferences were observed for creatinine, glucose, phosphate, protein and urate. For the lipaemic samples, interferences were observed for glucose, magnesium and urate, whilst for the haemolysed sample, potassium, creatinine, phosphate, magnesium, AST, ALT, CK, ALP, GGT, iron, TIBC, transferrin saturation were affected.

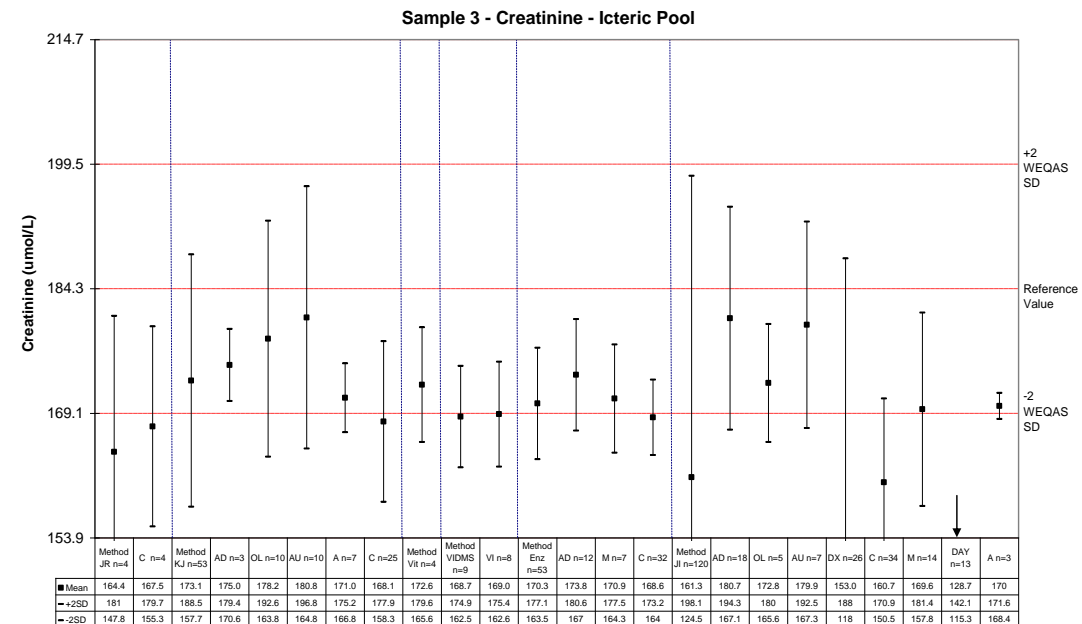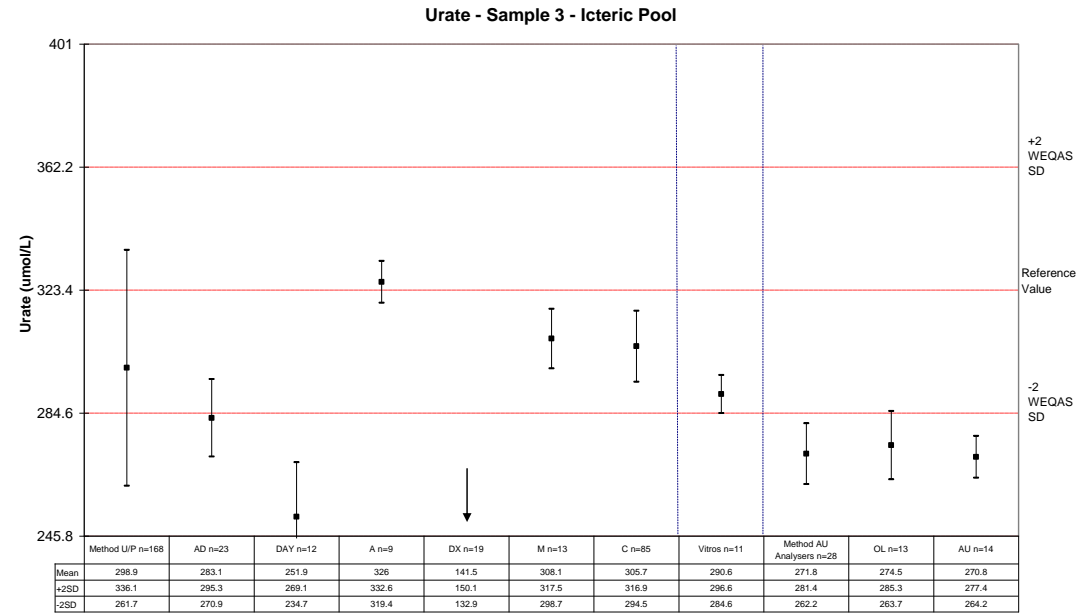


Identifying Assay Interferences – the Glick interforographs.


Graphical Comparisons of Interferences in Clinical Chemistry Instrumentation

Melvin R. Glick, Kenneth W. Ryder, and Sheila A. Jackson


Haemolysis

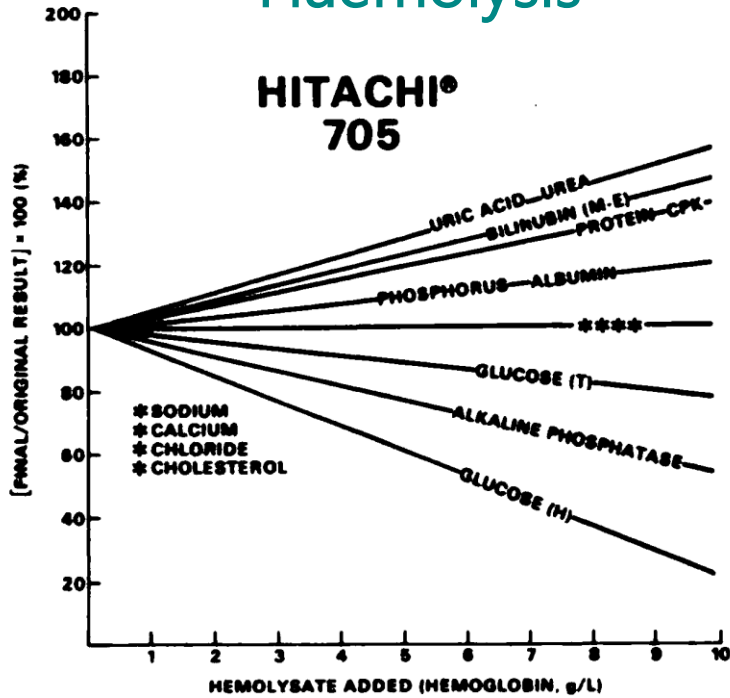

Lipaemia

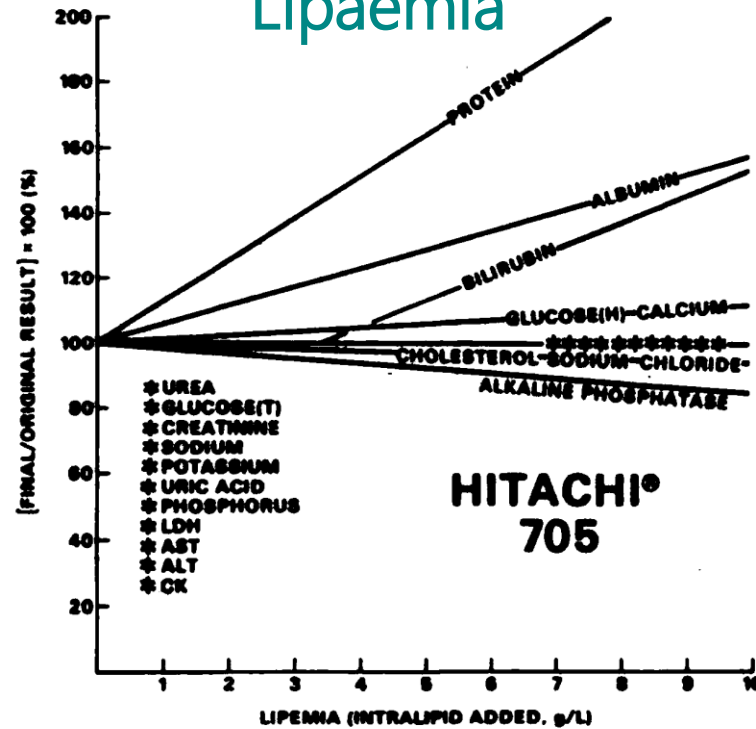

Icterus



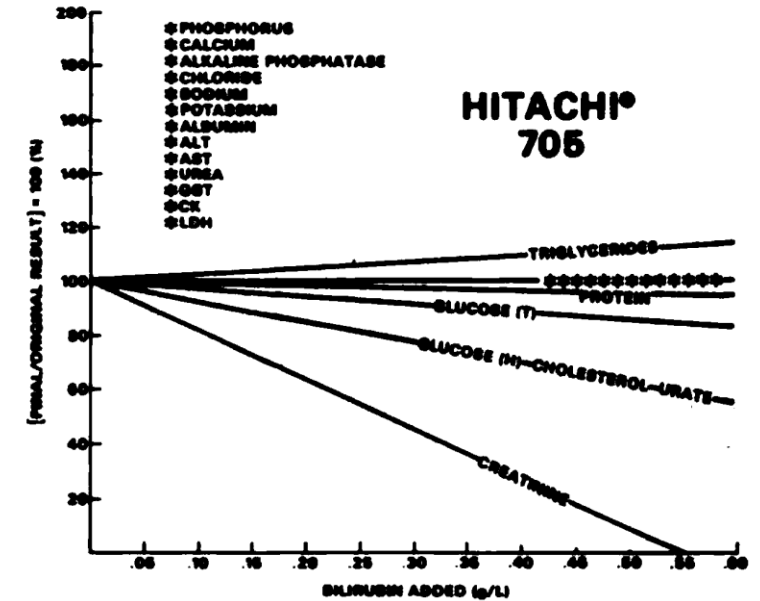


Pos effects on: UA, Urea, Bili, TP, CK, Alb, P.
Neg effects on: Glu, ALP

TP, Alb, Bili, Glu, Ca
Na, Cl, Chol, ALP




Trig
TP, Glu, Chol, UA, Creat

Olympus AU 500

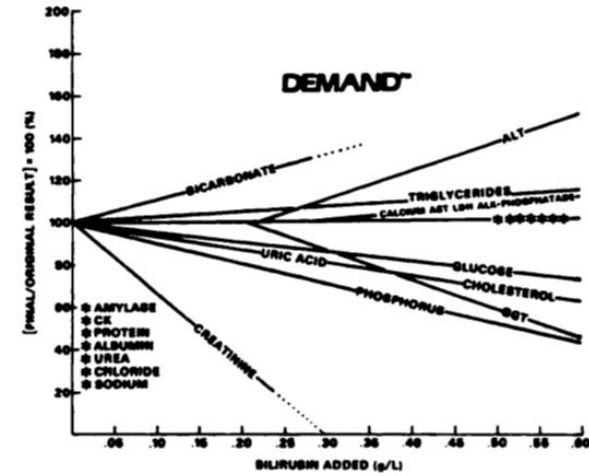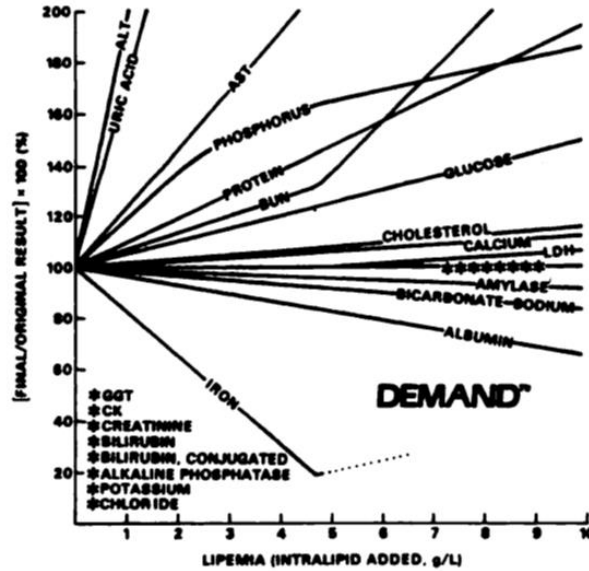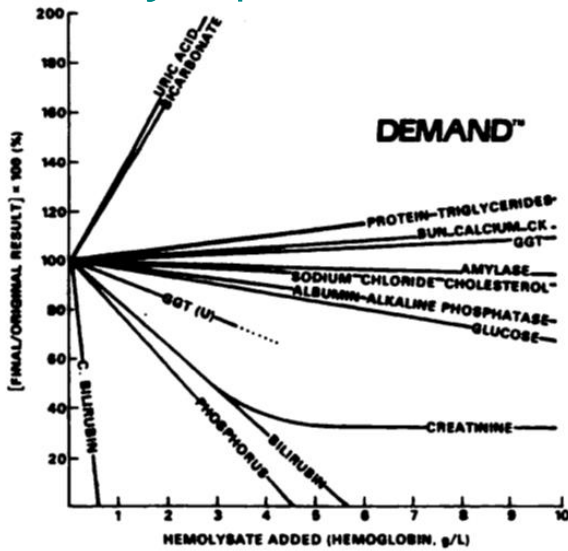

Large interference effects

Vitros dry slide technology

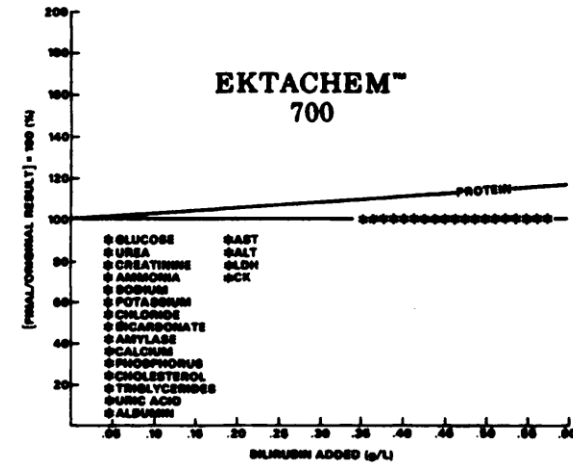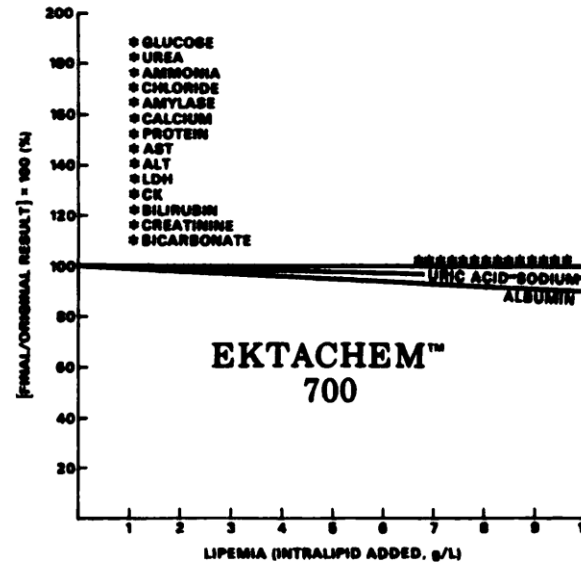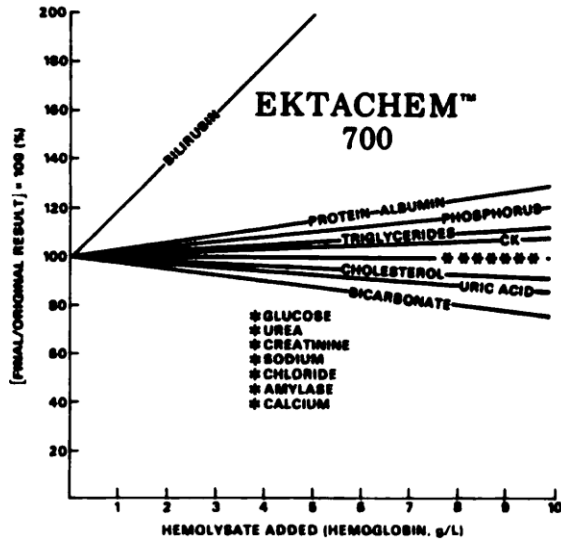


Minimal effects

Where are we now, 36 years later?

Icterus Interferograph

Weqas Data from 2012 to 2019

Percentage change in Results with Increasing Bilirubin Concentration

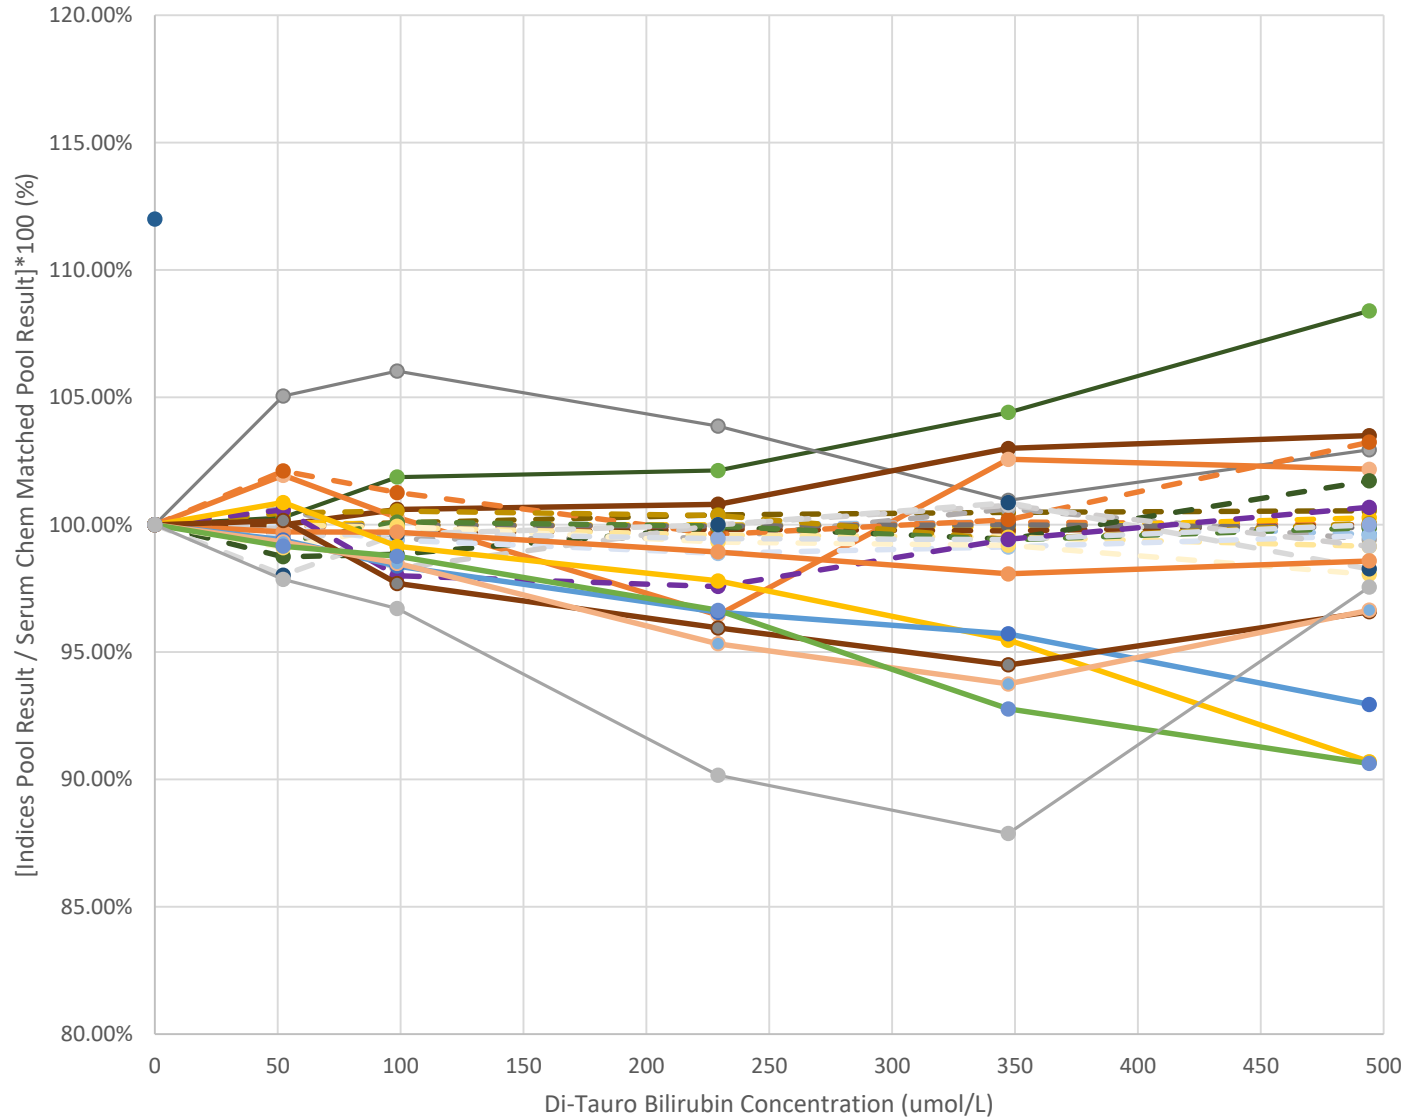


Pos effect


Neg effects

Weqas Data
from 2012 to
2019


Percentage change in Results with Increasing Bilirubin Concentration

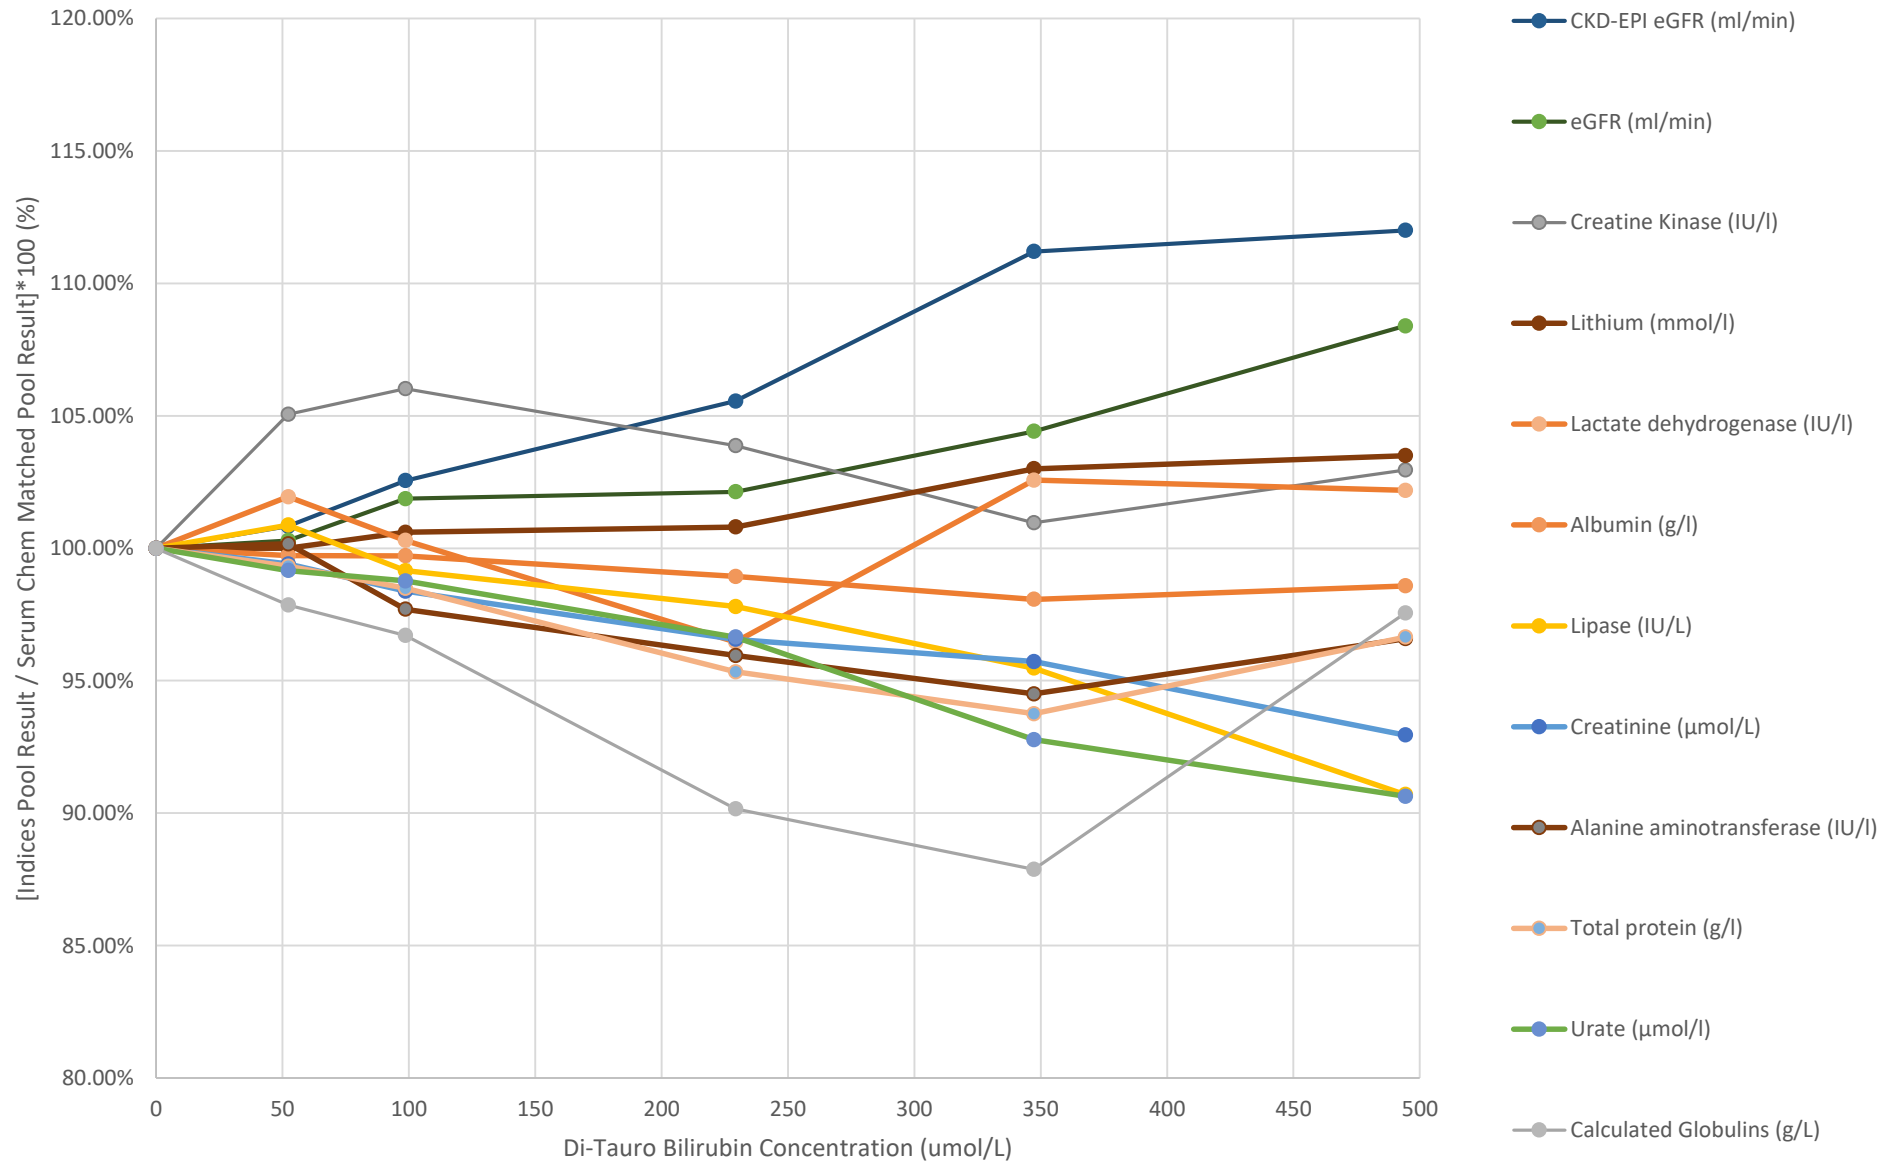

Percentage change in Results with Increasing Bilirubin Concentration

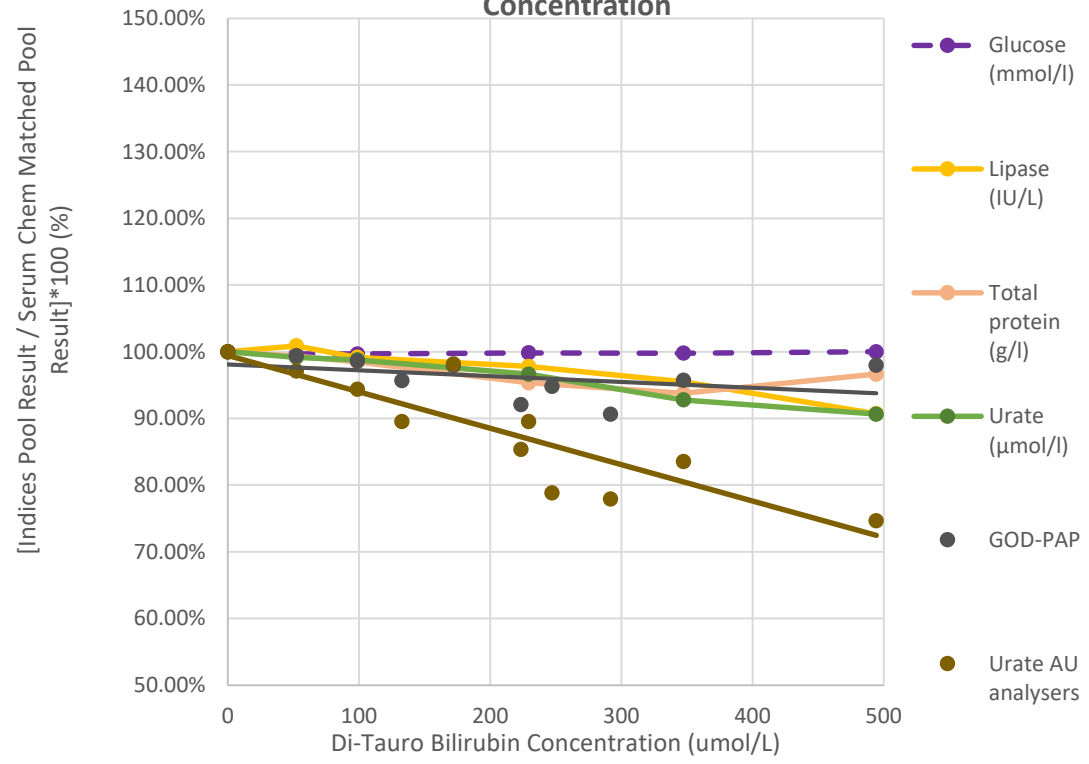


Percentage change in Creatinine Results with Increasing Bilirubin Concentration

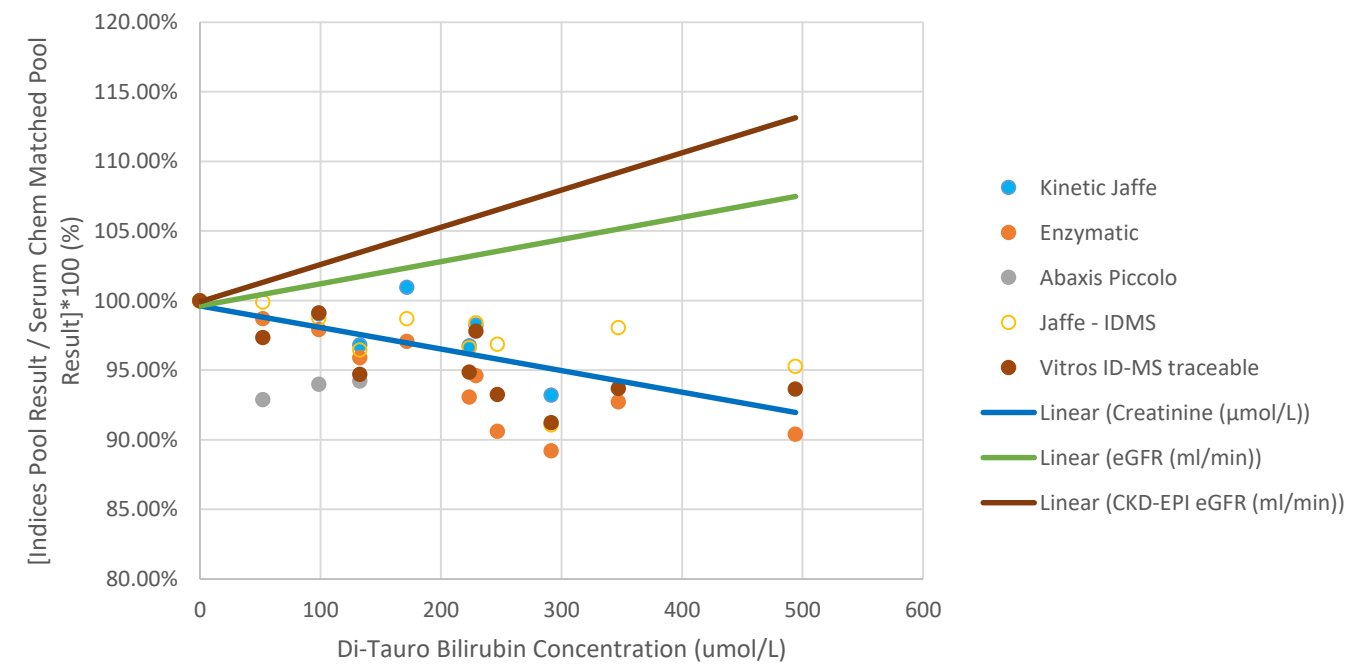

Icterus Interferograph

Interference effects for Urate by analyser

Weqas Data
2019- 2022

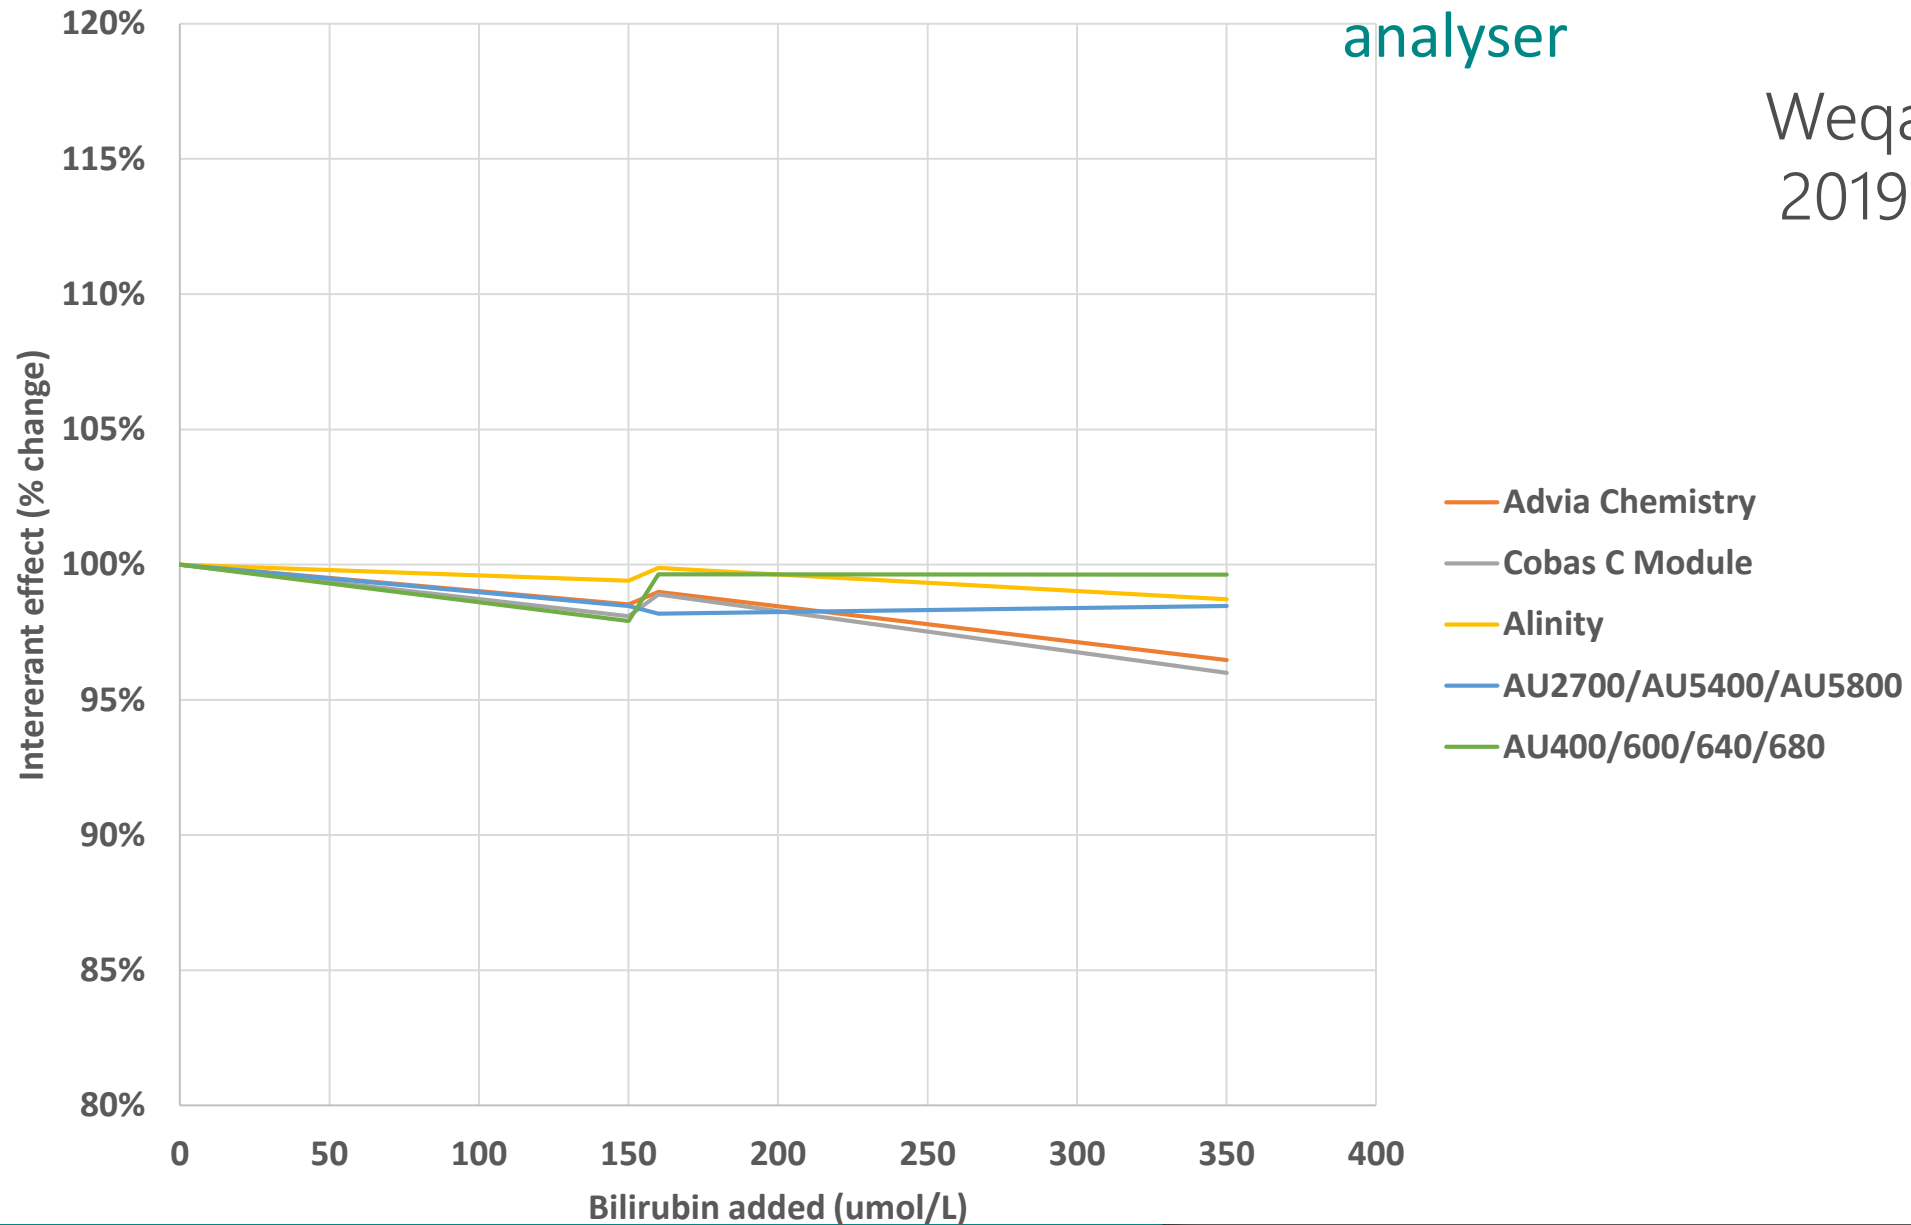


Haemolysis Interferograph


Weqas Data
from 2012 to
2018

Analytes where little or no effect observed

Percentage change in Results with Increasing Haemolysis Effect

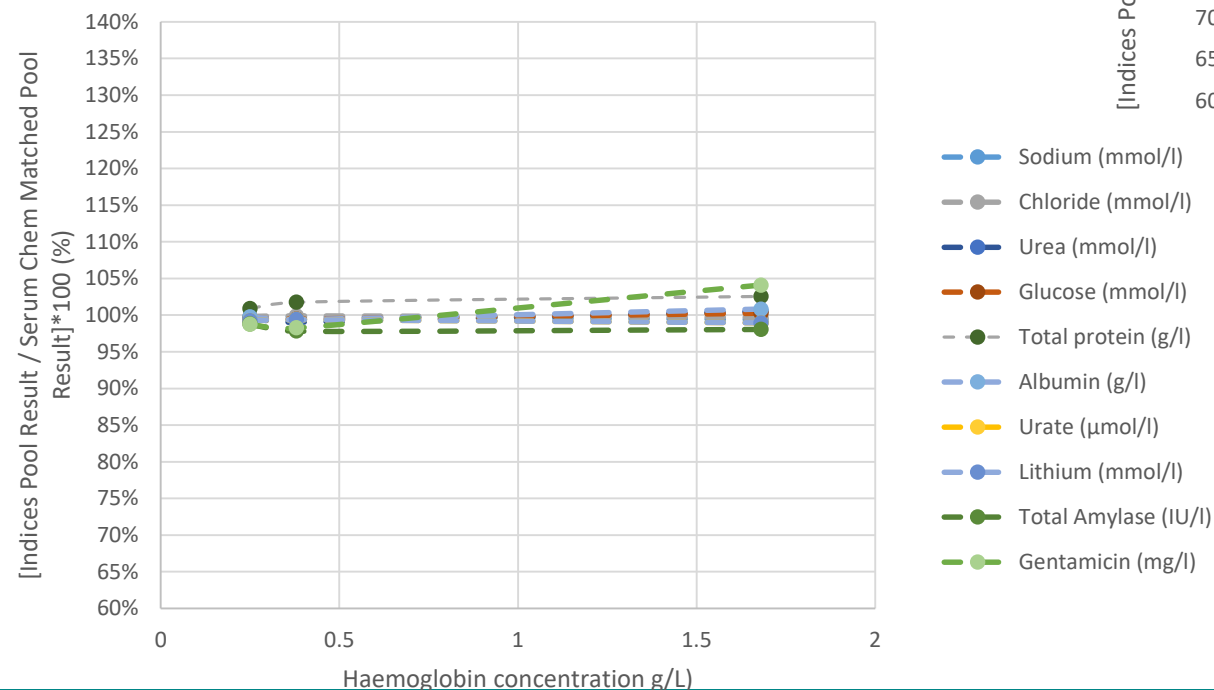


Percentage change in Results with Increasing Haemolysis Effect

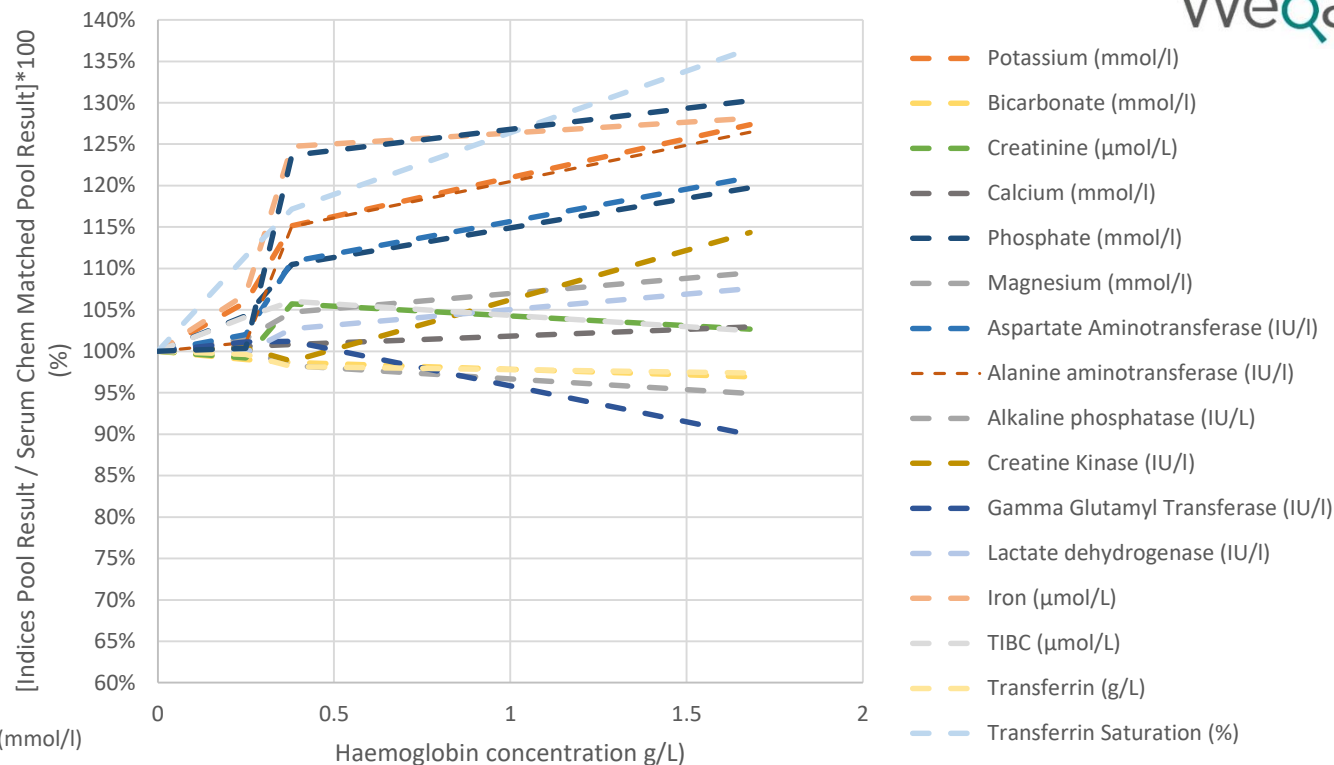


	Analytes affected by Interferant	
	Positive	Negative
Pos (RBC)	Lipase, ALT	GGT
Iron	CK	ALP
K	Mg, LDH	Transferrin
AST, P	Creat, TiBC	

Haemolysis Interferograph

Weqas Data
2019- 2022

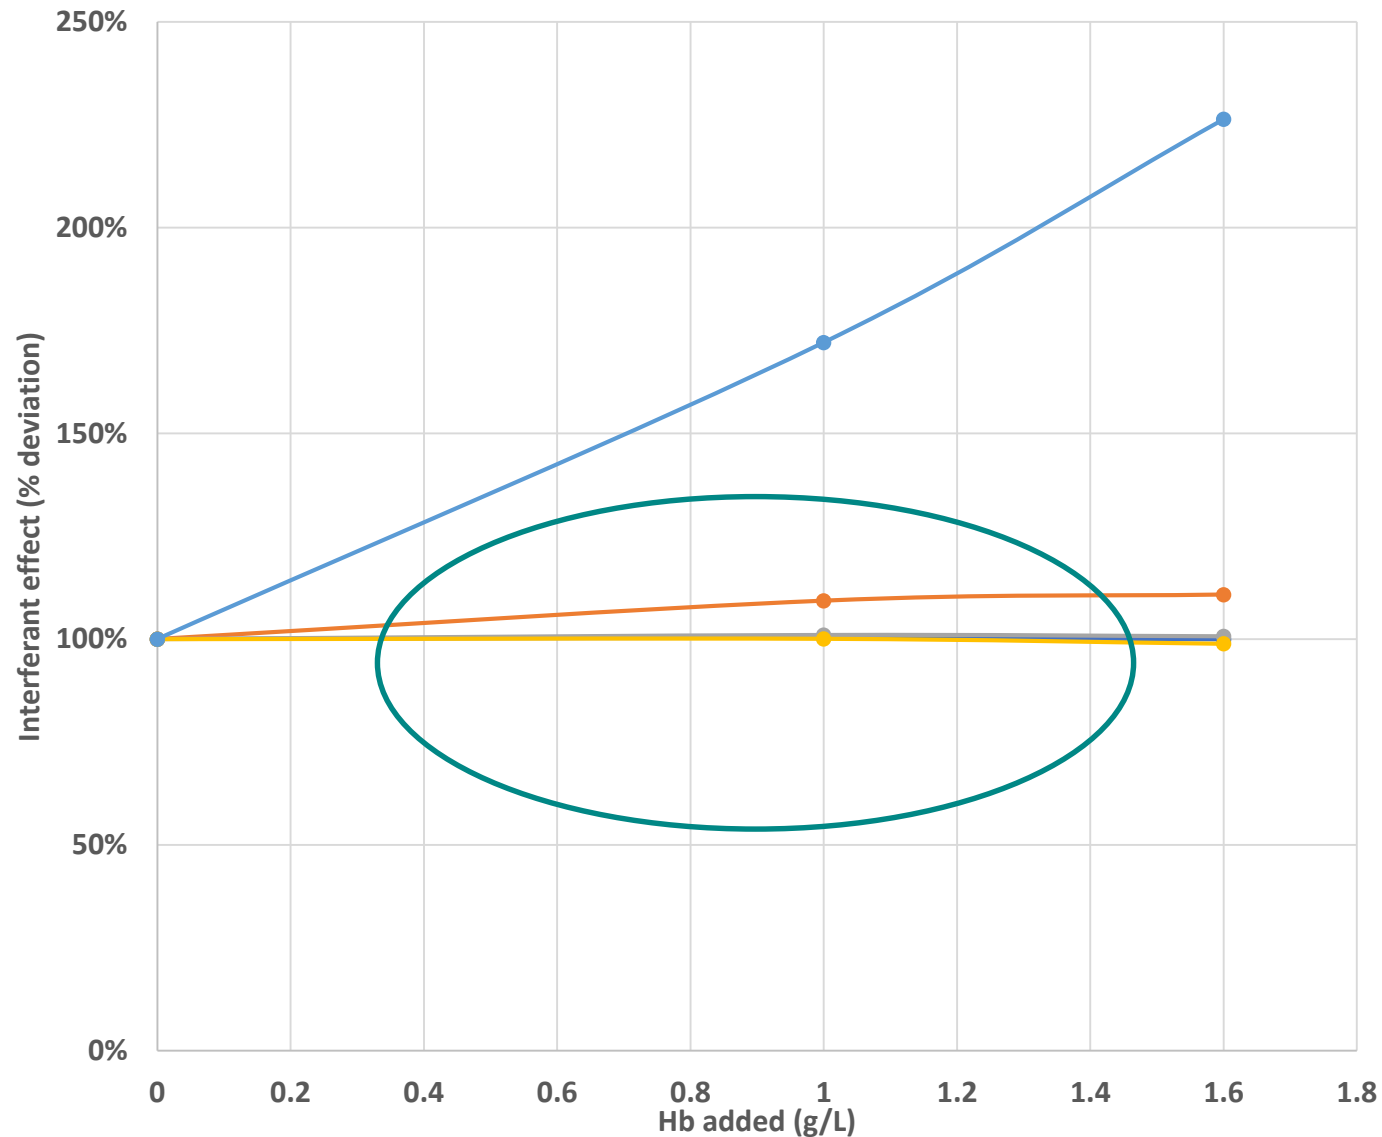

- Sodium (mmol/l)
- Potassium (mmol/l)
- Creatinine (µmol/L)
- Alanine Aminotransferase (IU/l)
- Lactate dehydrogenase (IU/l)

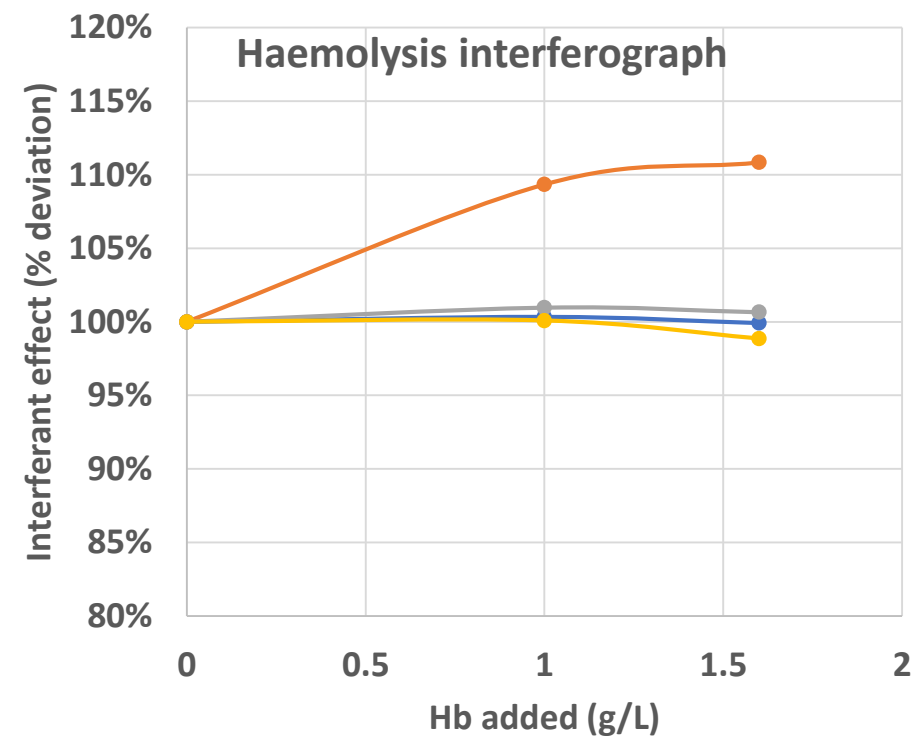

Lipaemia Interferograph

Weqas Data from 2012 to 2019

Analytes where little or no effect observed

